


ECG PARA EL FORUM

SEPTAL WITH qWAVE

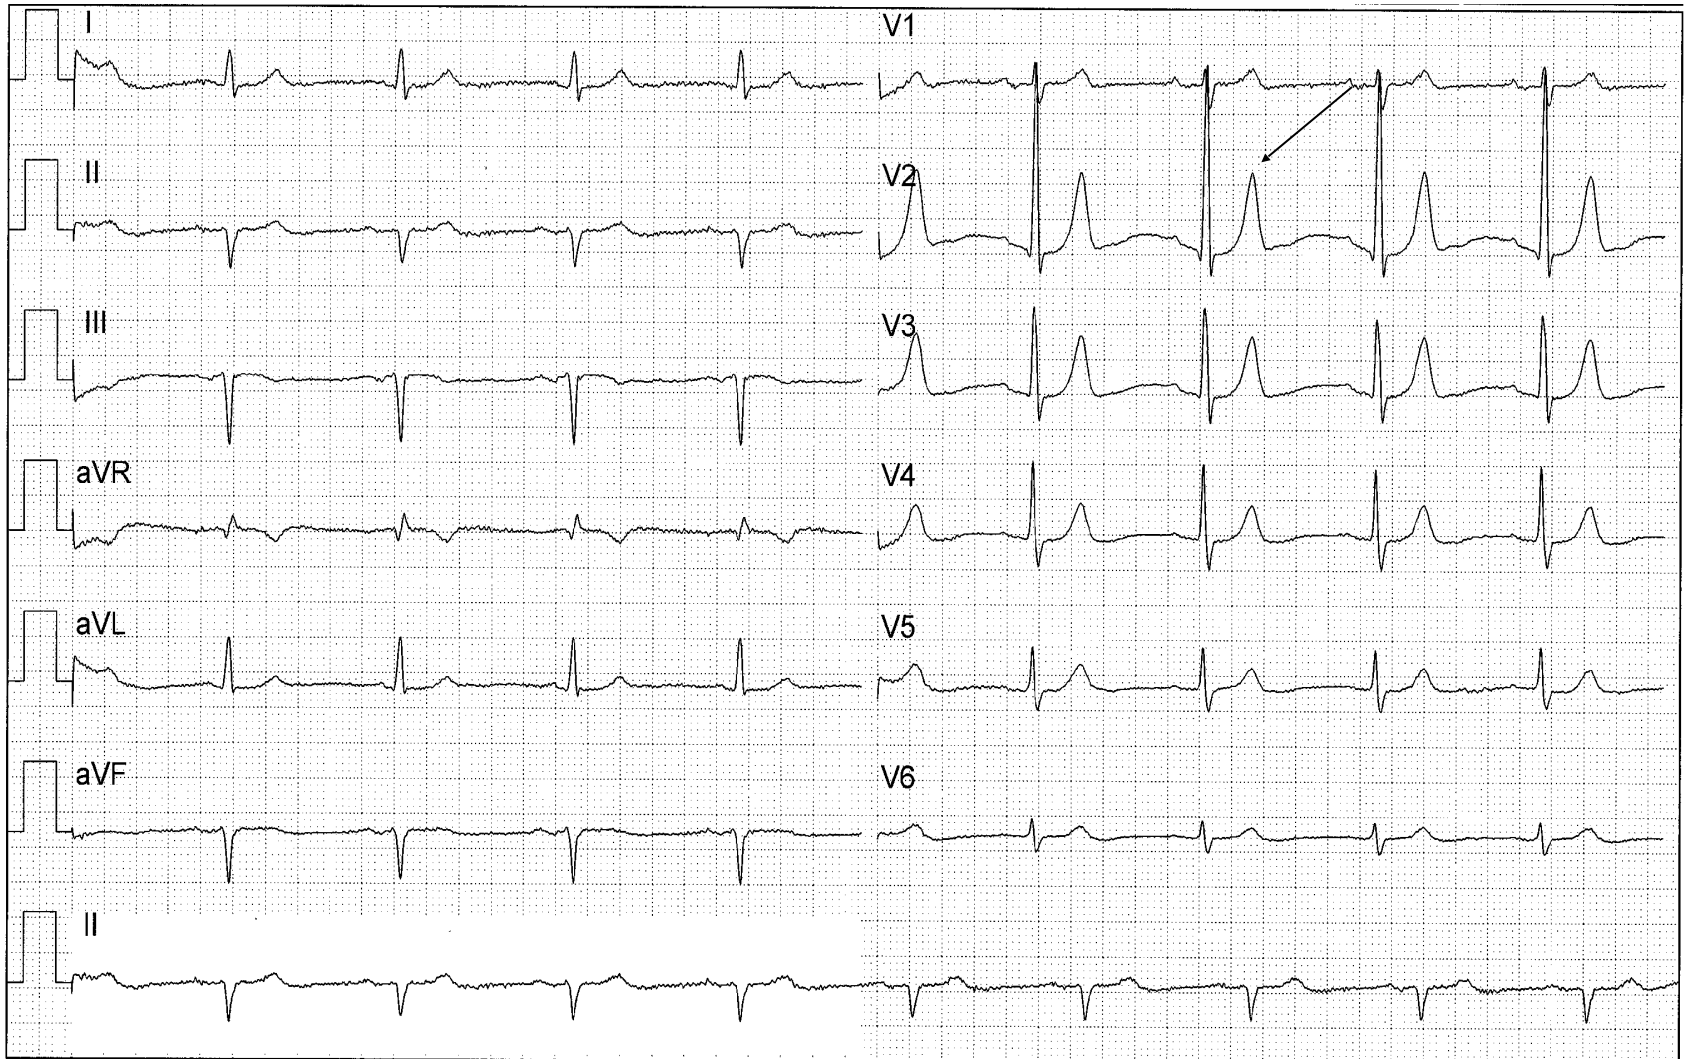

25 mm/sec 10 mm/mV Filters: 50 Hz -on; BL -on; 0.05-40 Hz

May 18, 2006 09:16

Norav Medical Ltd. rev. 4. 5. 765


N 16 – S A – 313931248 – 82 – F – HT

SEPTAL NO q WAVE



KM, 307572743, F, 84,

SEPTAL q WAVE V2

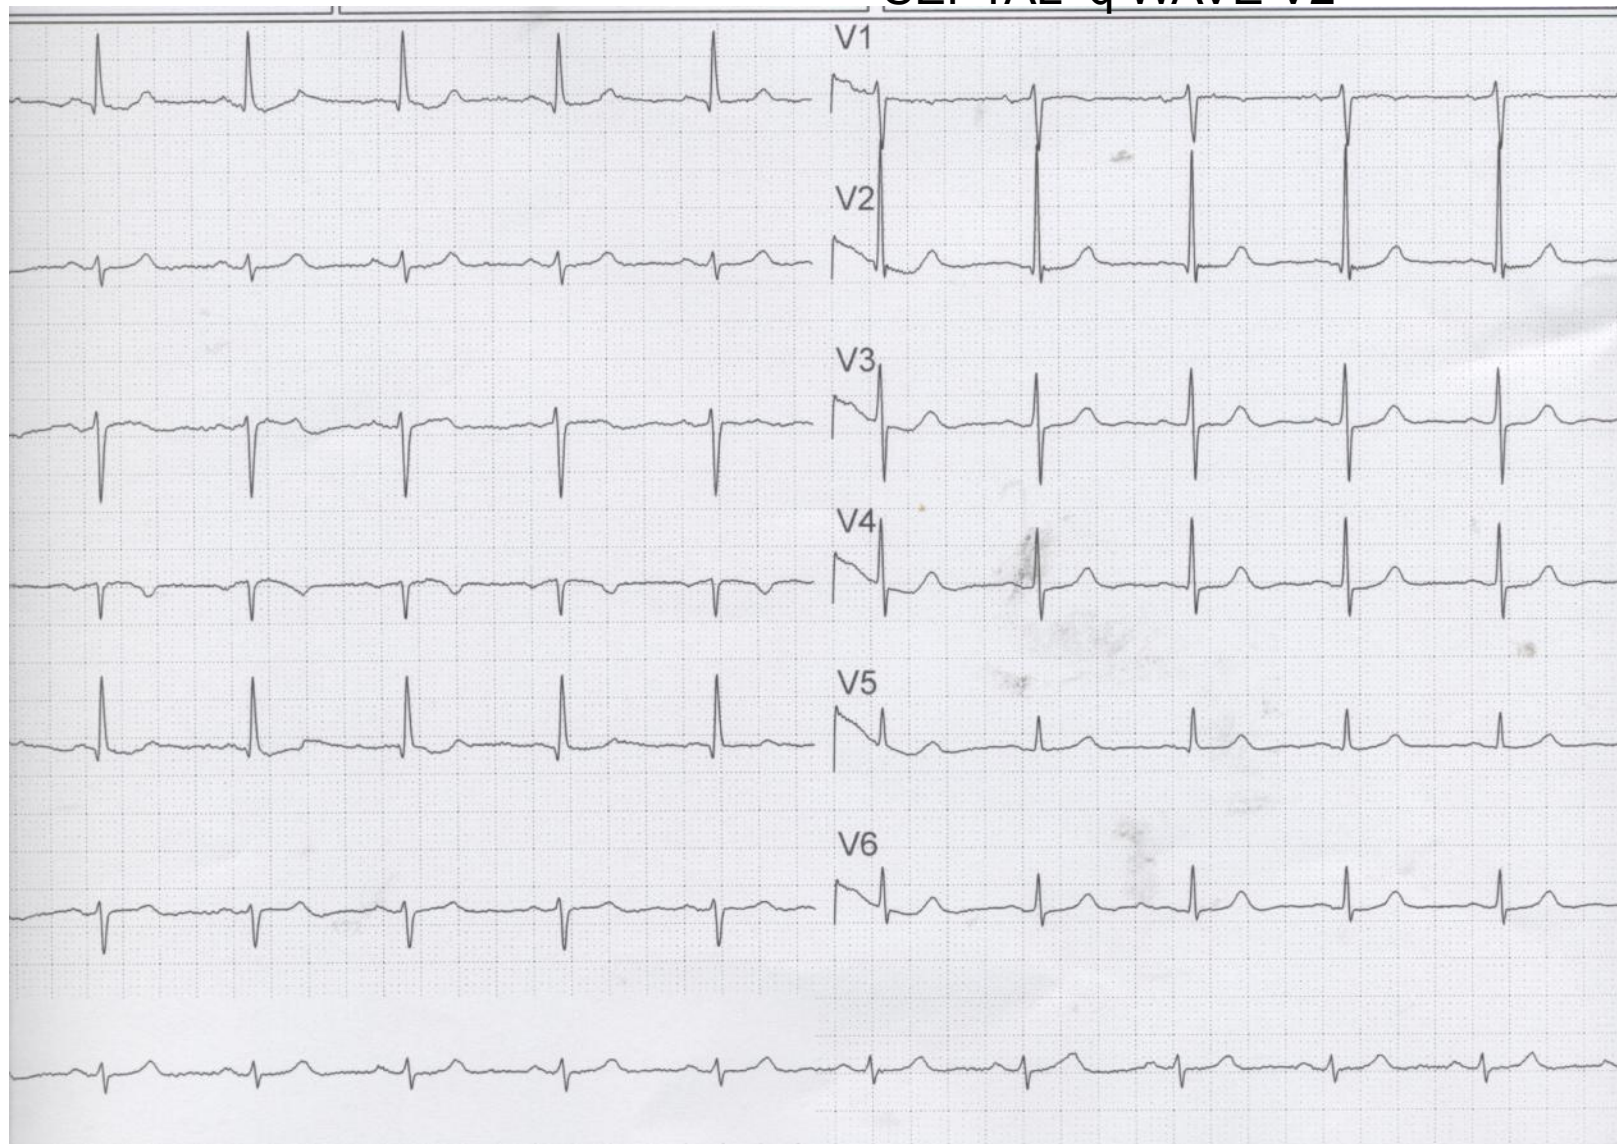


mm/mV Filters: 50 Hz -on; BL -on; 0.05-40 Hz


January 27, 2008 10:44

Norav Medical Ltd

N48,SHM, 030233035, M, 72,

septal sin q

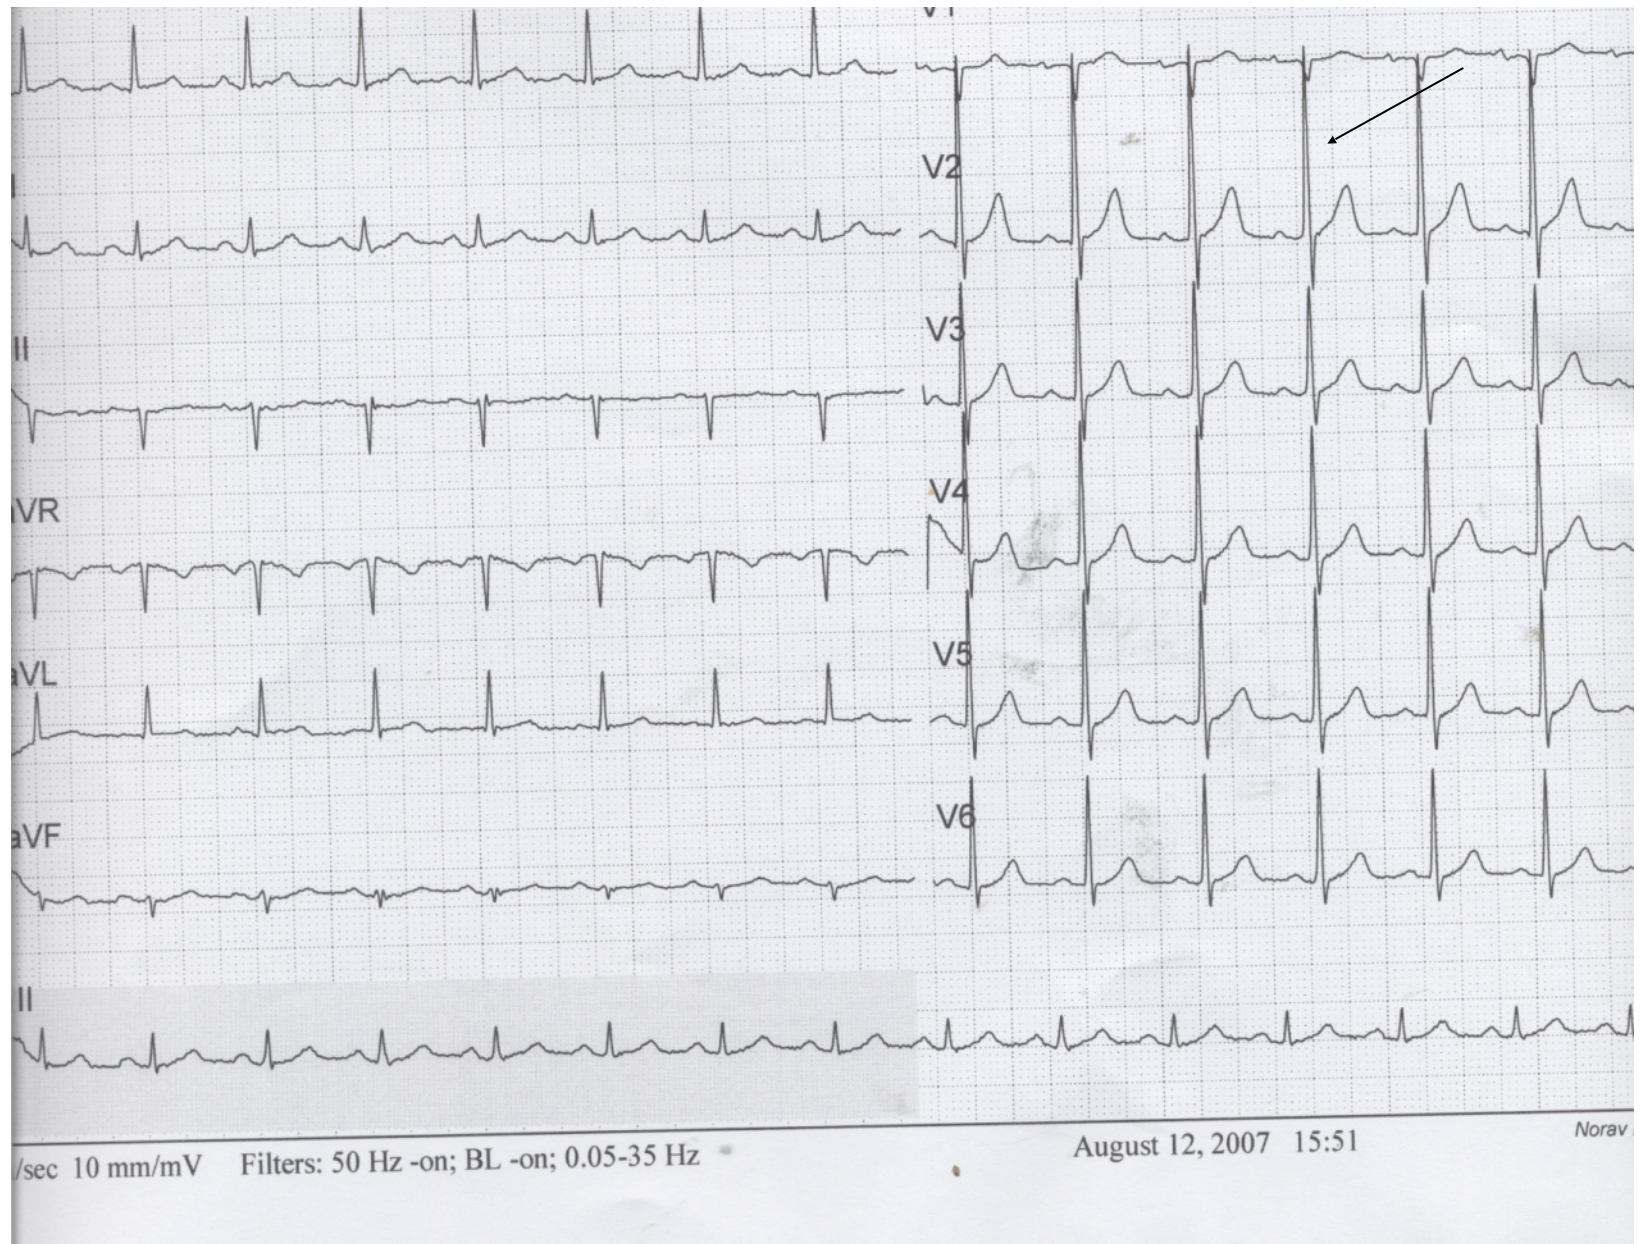

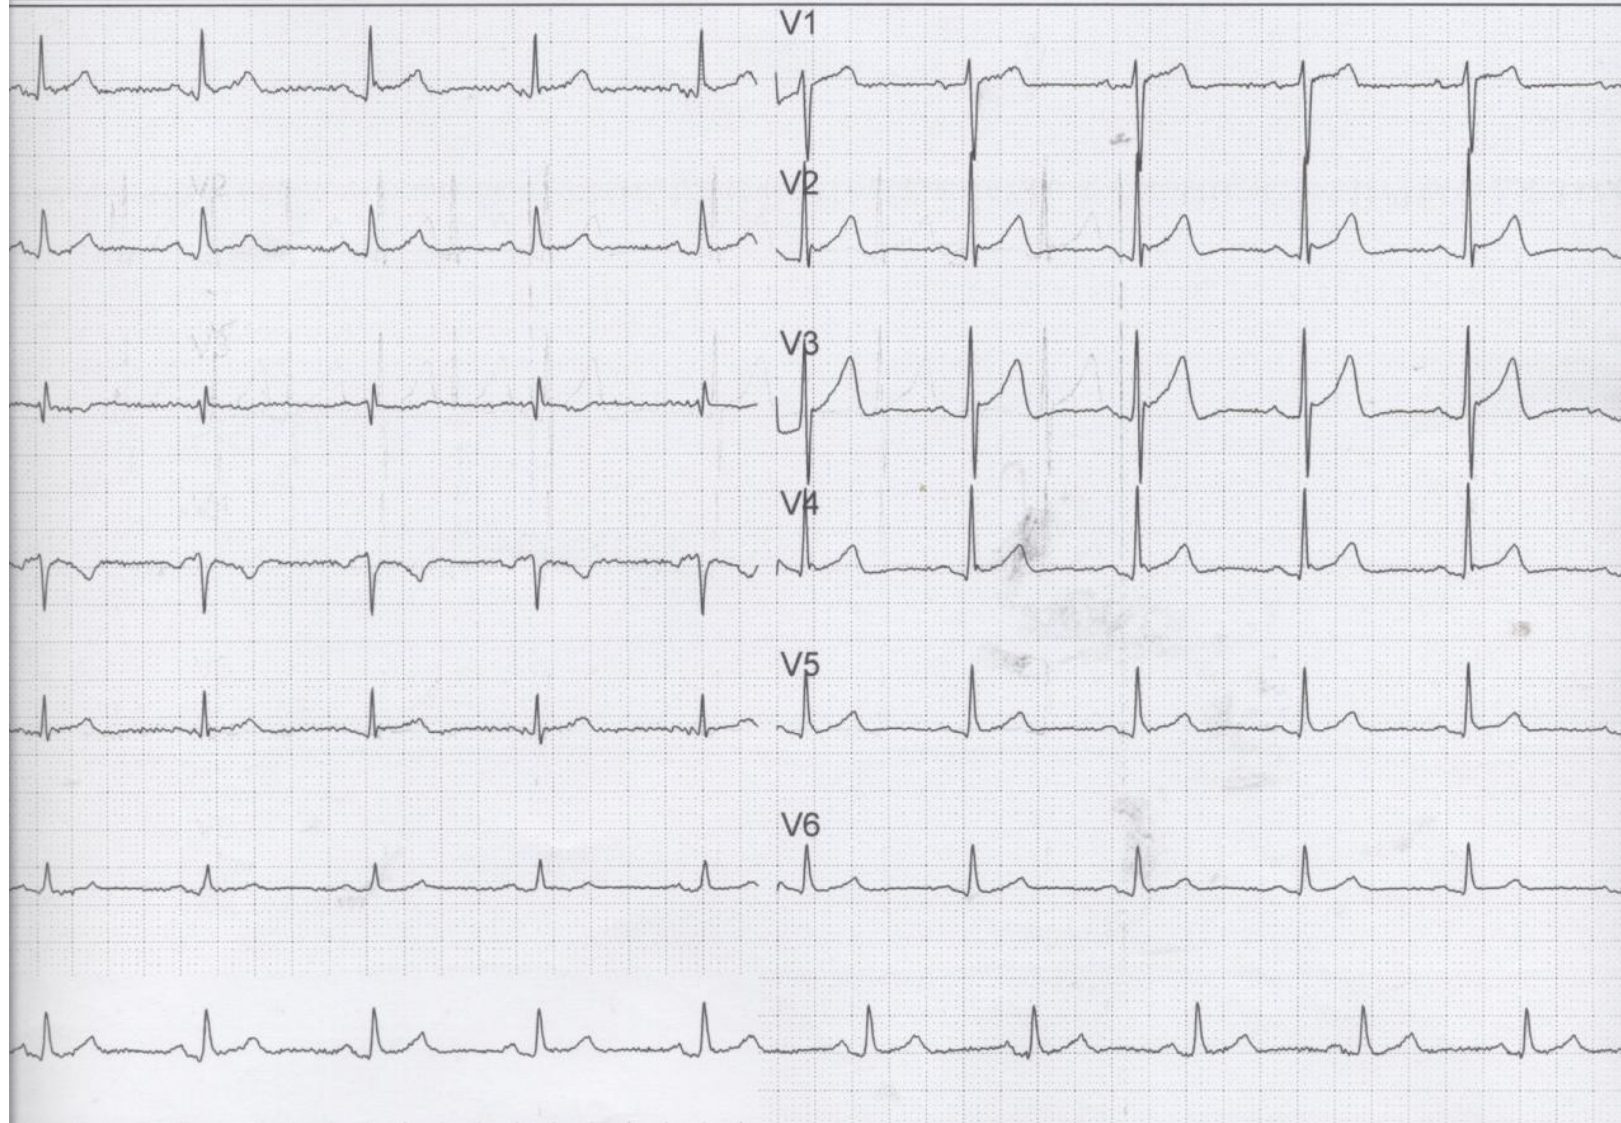


mV Filters: 50 Hz -on; BL -on; 0.05-40 Hz

December 18, 2007 08:53

Norav Medical Ltd. rev. 4

HF, 068484419, F, 75, HT, DM septal sin q

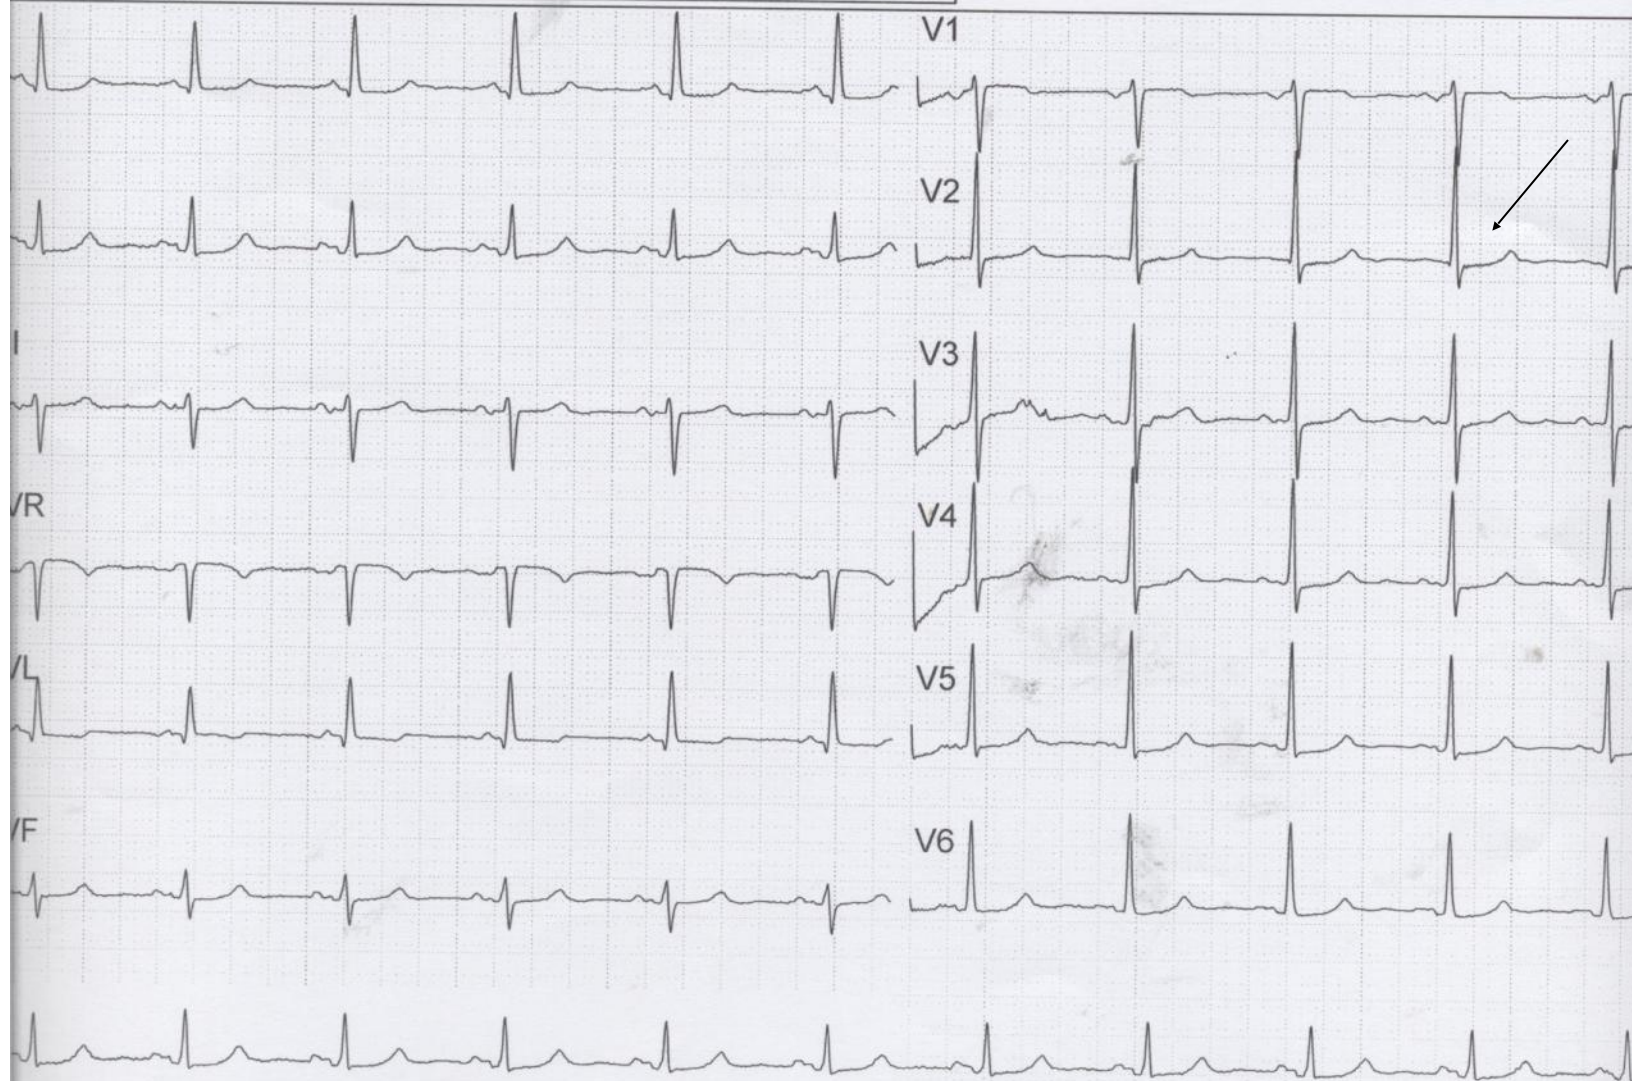


c 10 mm/mV Filters: 50 Hz -on; BL -on; 0.05-40 Hz

February 03, 2008 10:03


Norav Medi

Septal sin q

N 1 – G G – 007906795 –76 – M

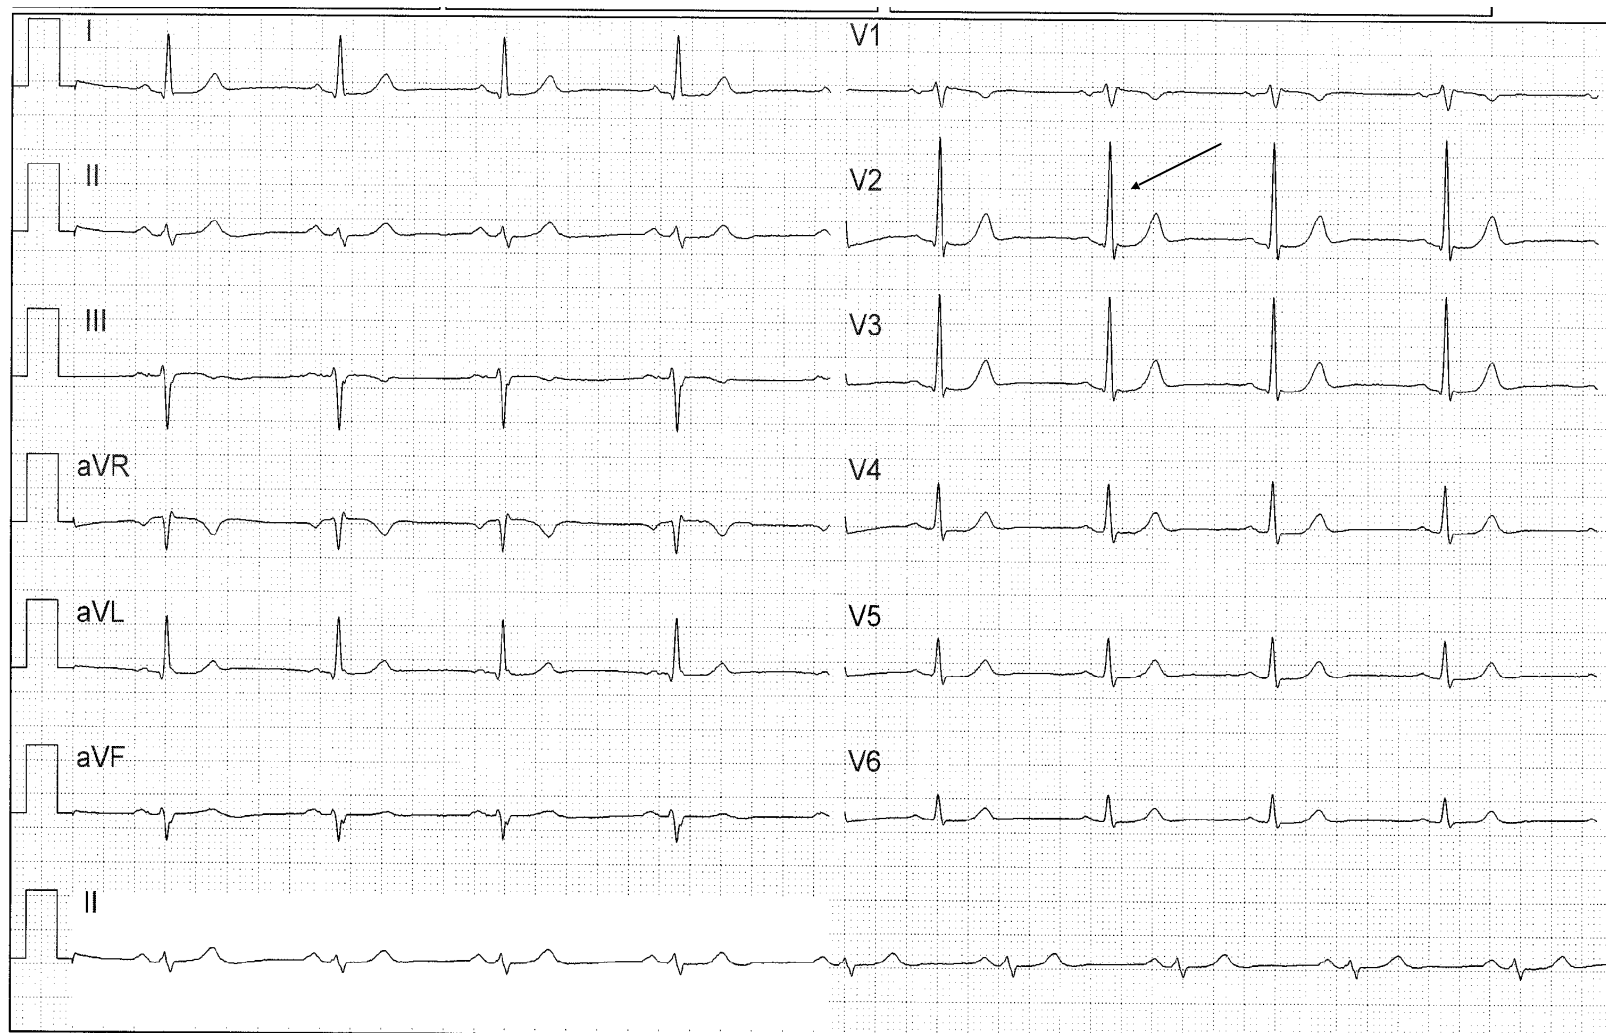

AE, 55209,M,82,AF,HT apical

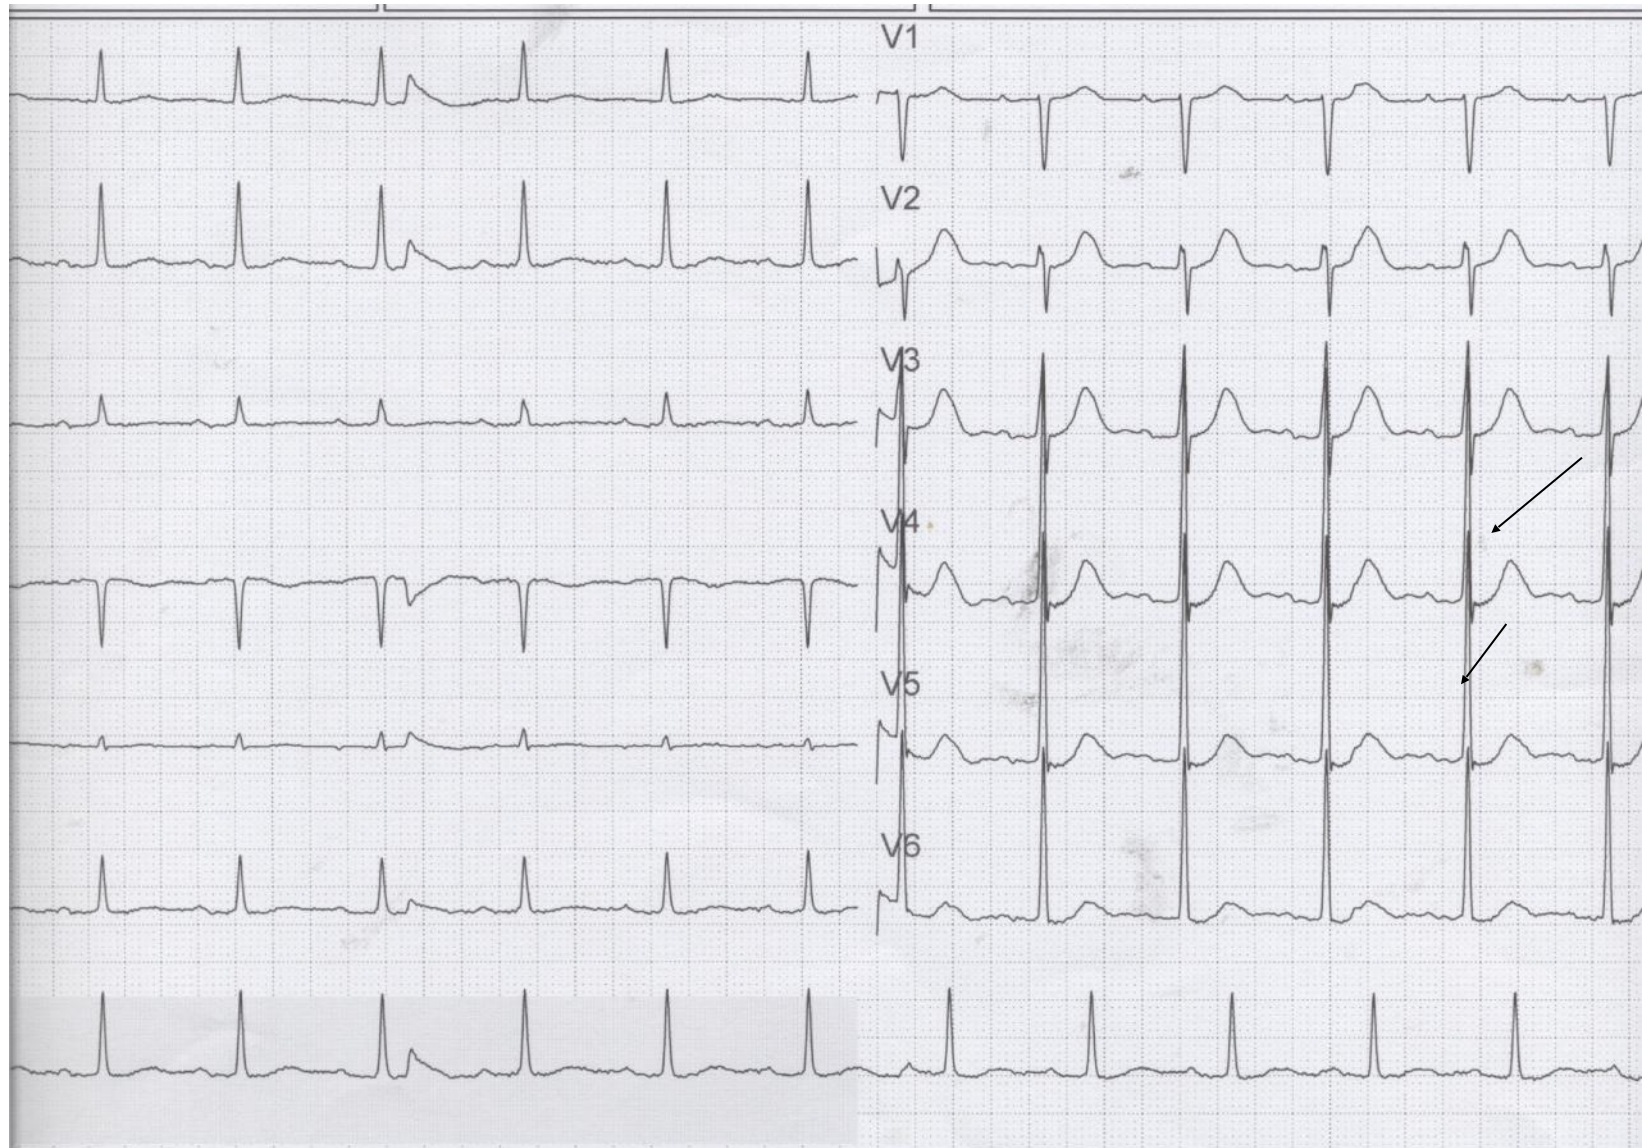


10 mm/mV Filters: 50 Hz -on; BL -on; 0.05-35 Hz


January 23, 2008 11:42

Norav Medical


El mismo caso

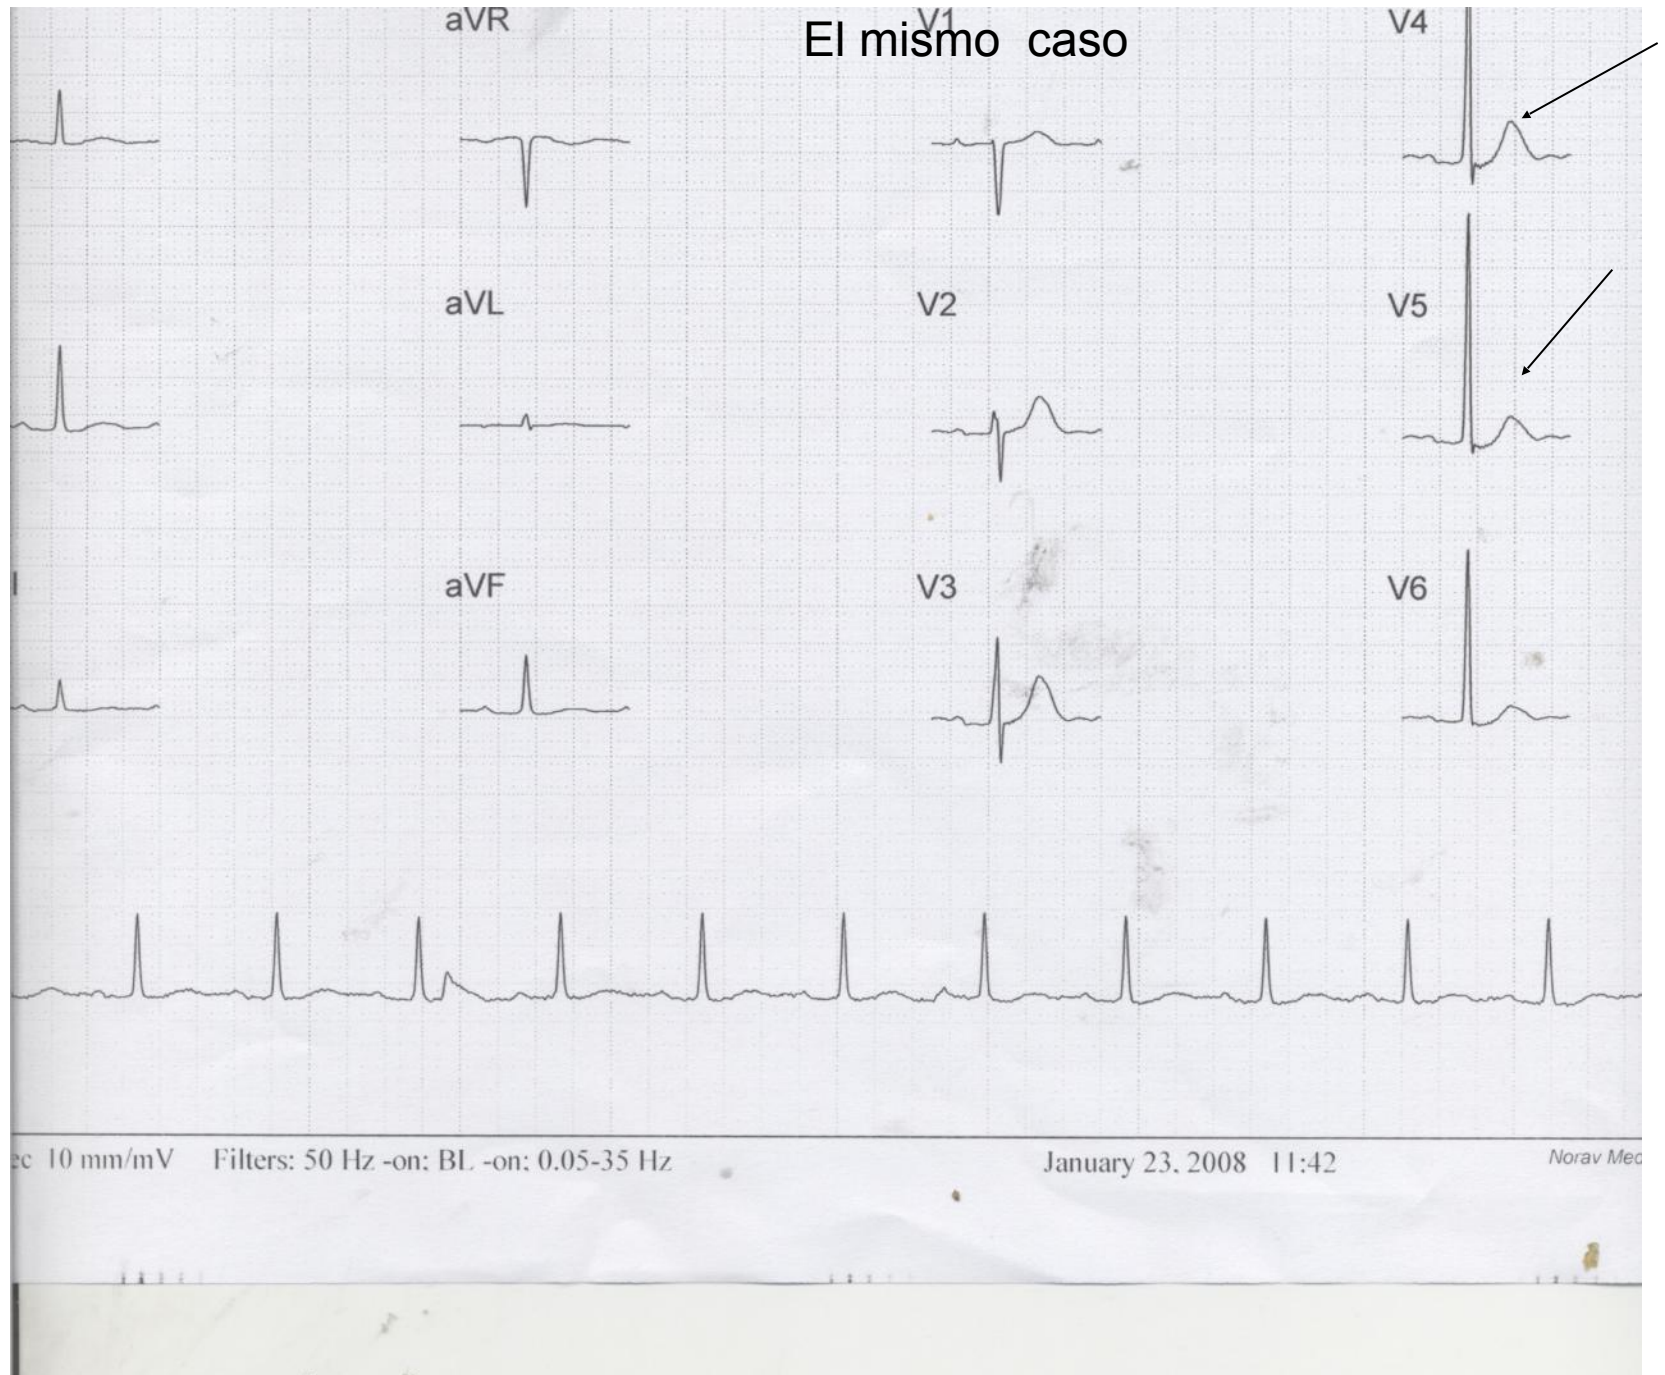

apical

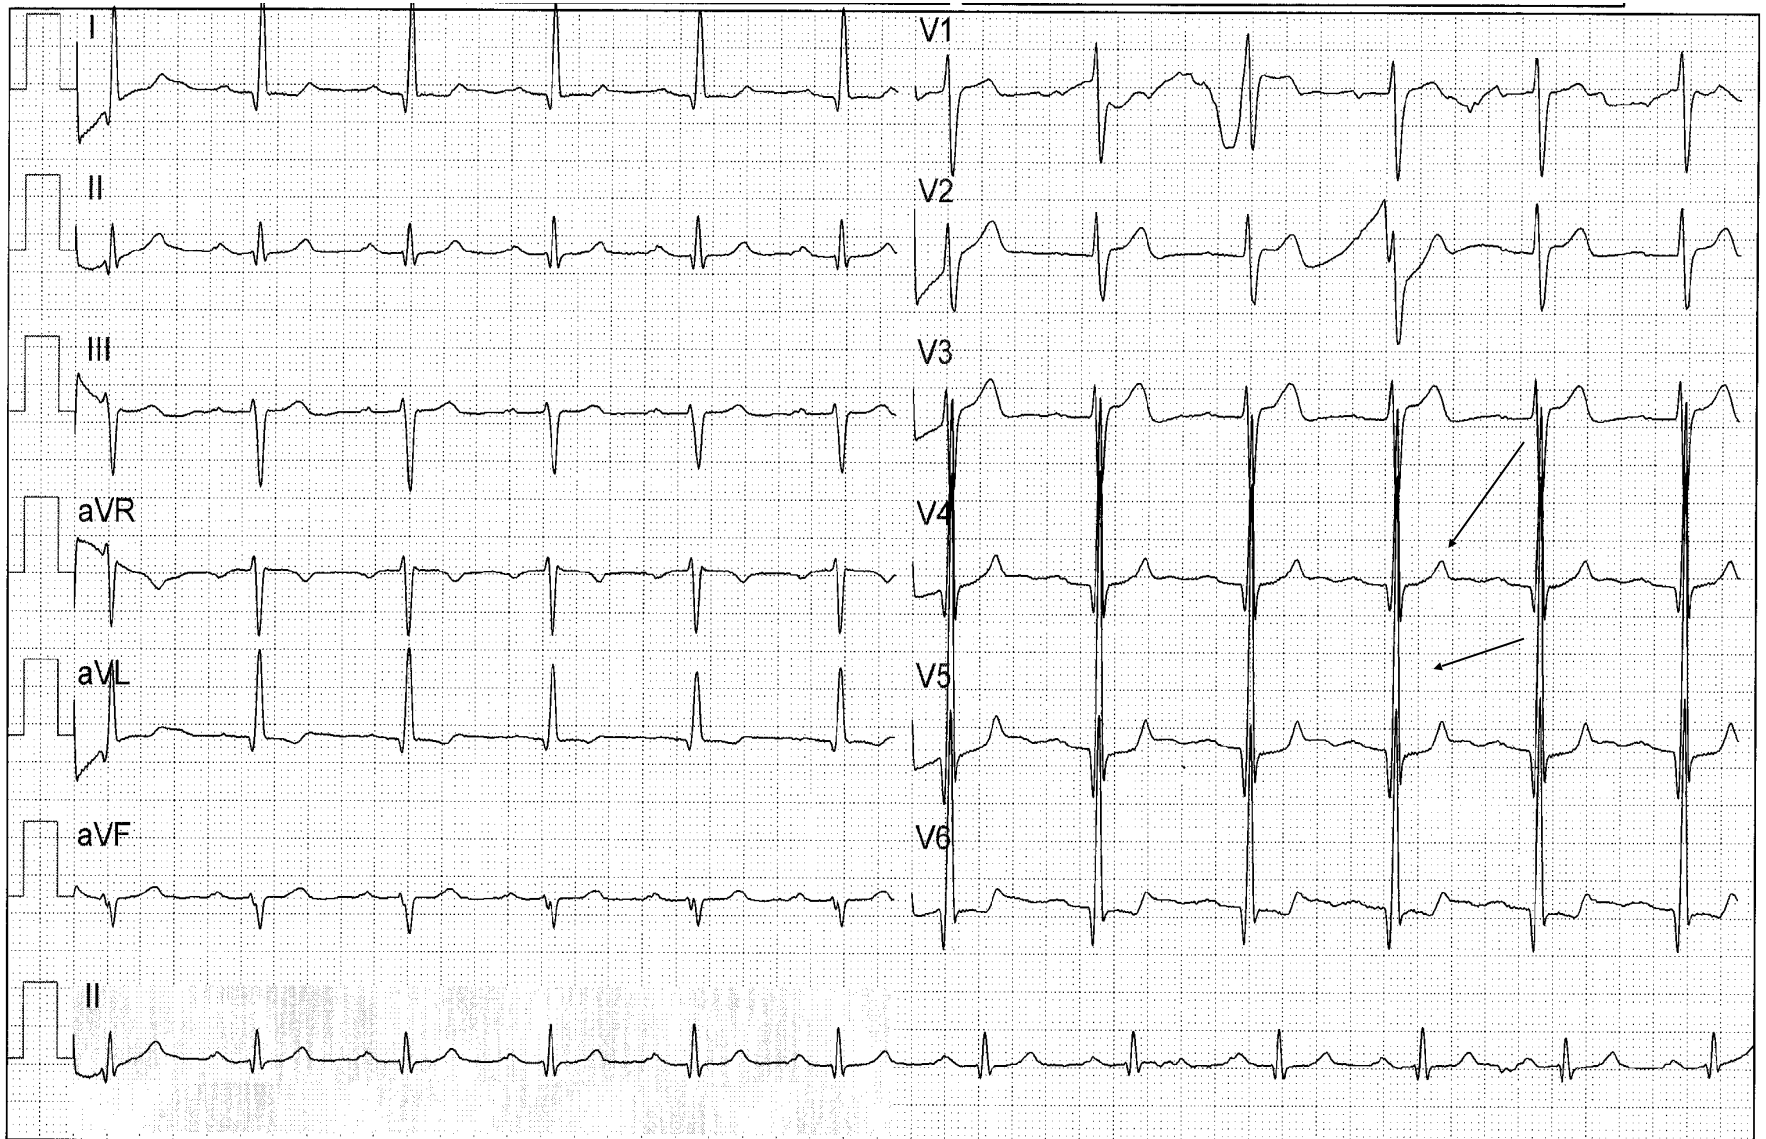

El mismo caso

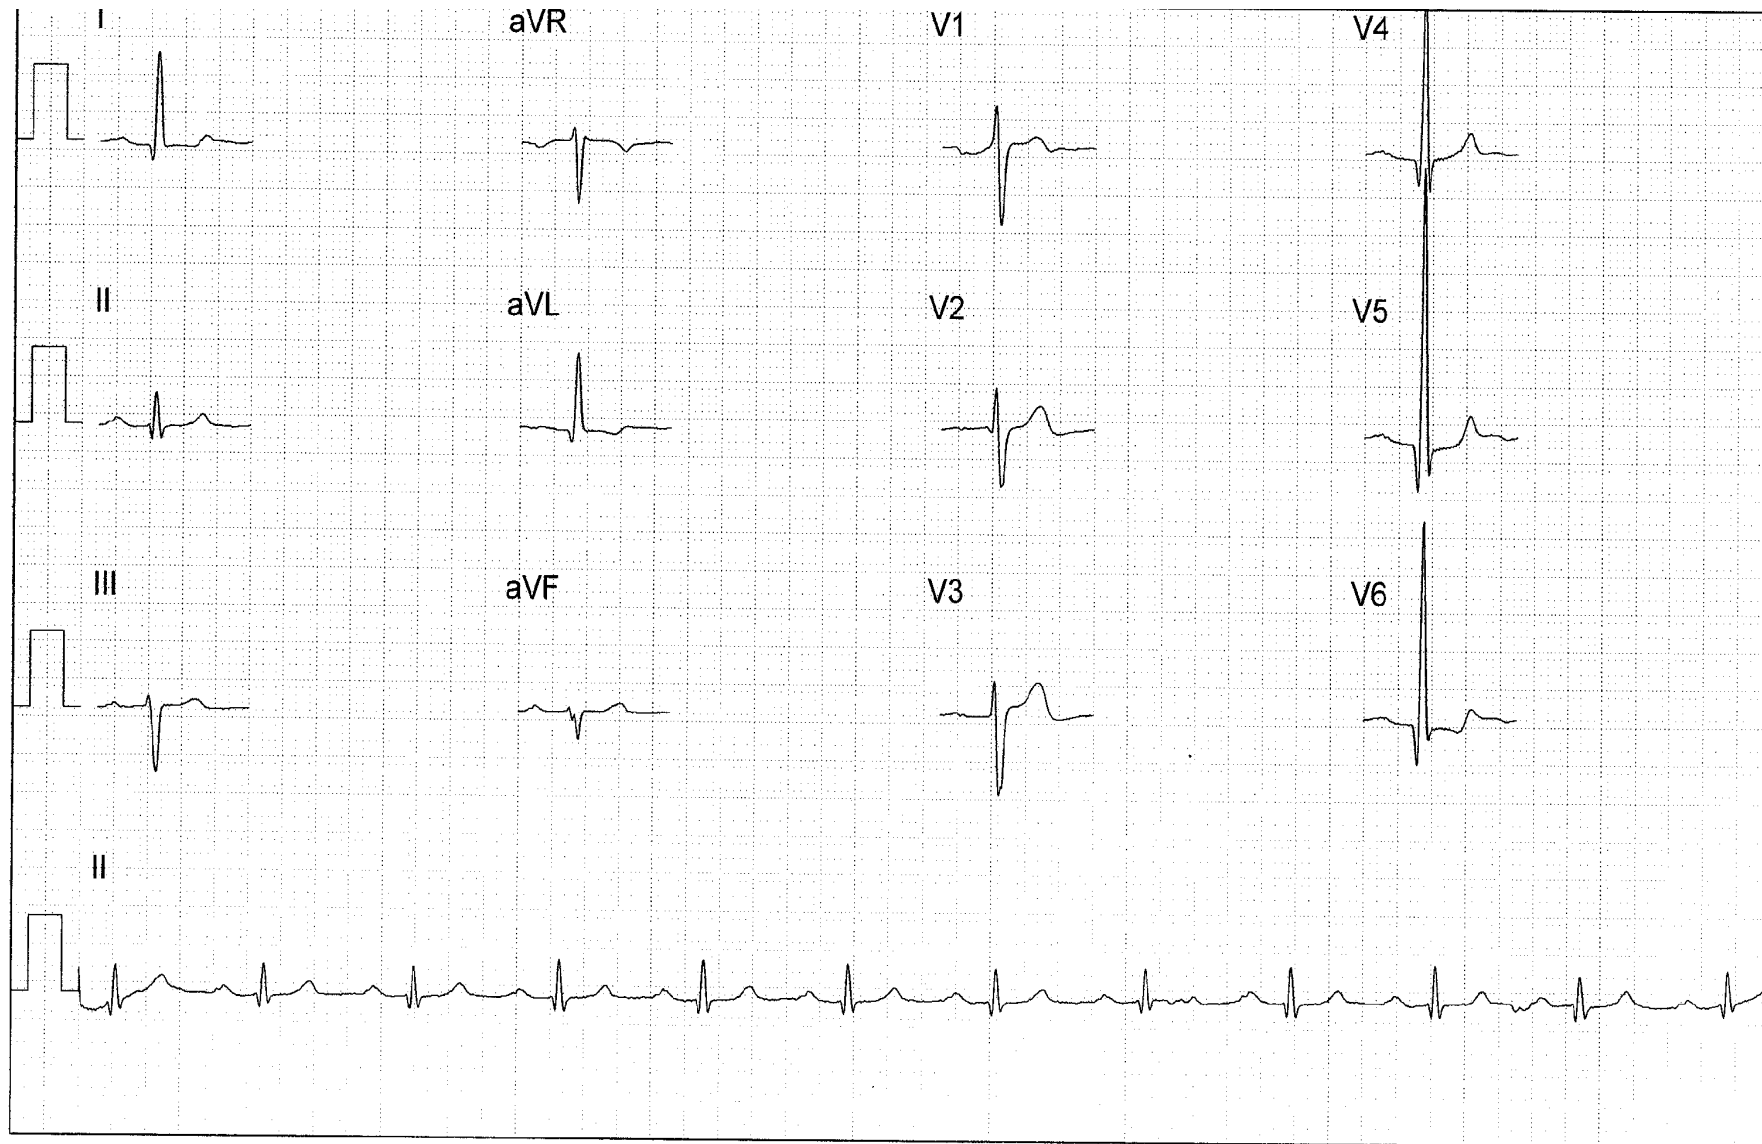

25 mm/sec 10 mm/mV Filters: 50 Hz -on; BL -on; 0.05-35 Hz


January 28, 2008 08:49

Norav Medical Ltd. rev. 4. 5. 765

Birth Date: 07/03/1923 Age: 84

Sex: F

basal

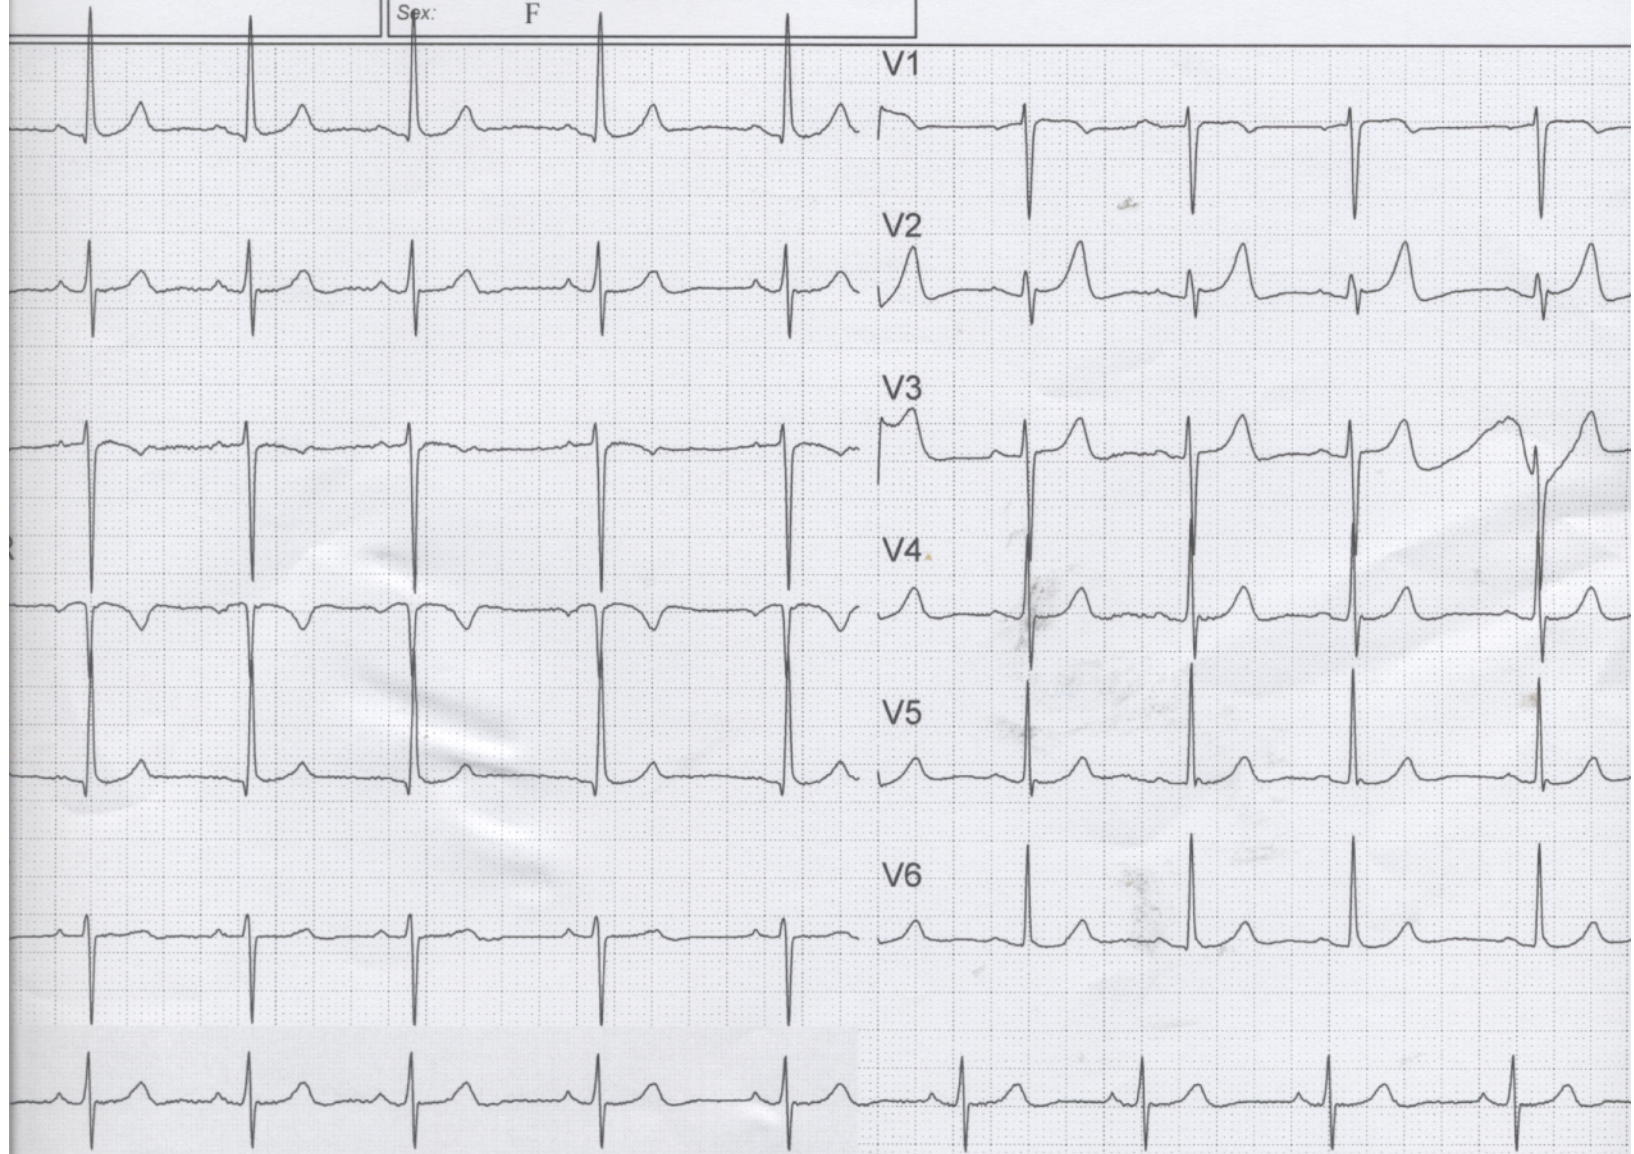

10 mm/mV Filters: 50 Hz -on; BL -on; 0.05-35 Hz

May 06, 2007 08:09

Norav Medical

Birth Date: 07/03/1923 Age: 84

Sex: F

N 6- MI-9453-81- M-

basal

CVA,, HT

V1

V2

V3

V4

V5

V6


10 mm/mV Filters: 50 Hz -on; BL -on; 0.05-35 Hz

May 06, 2007 08:09

Norav Medical

N39,KR7228,F,85,HT

lateral

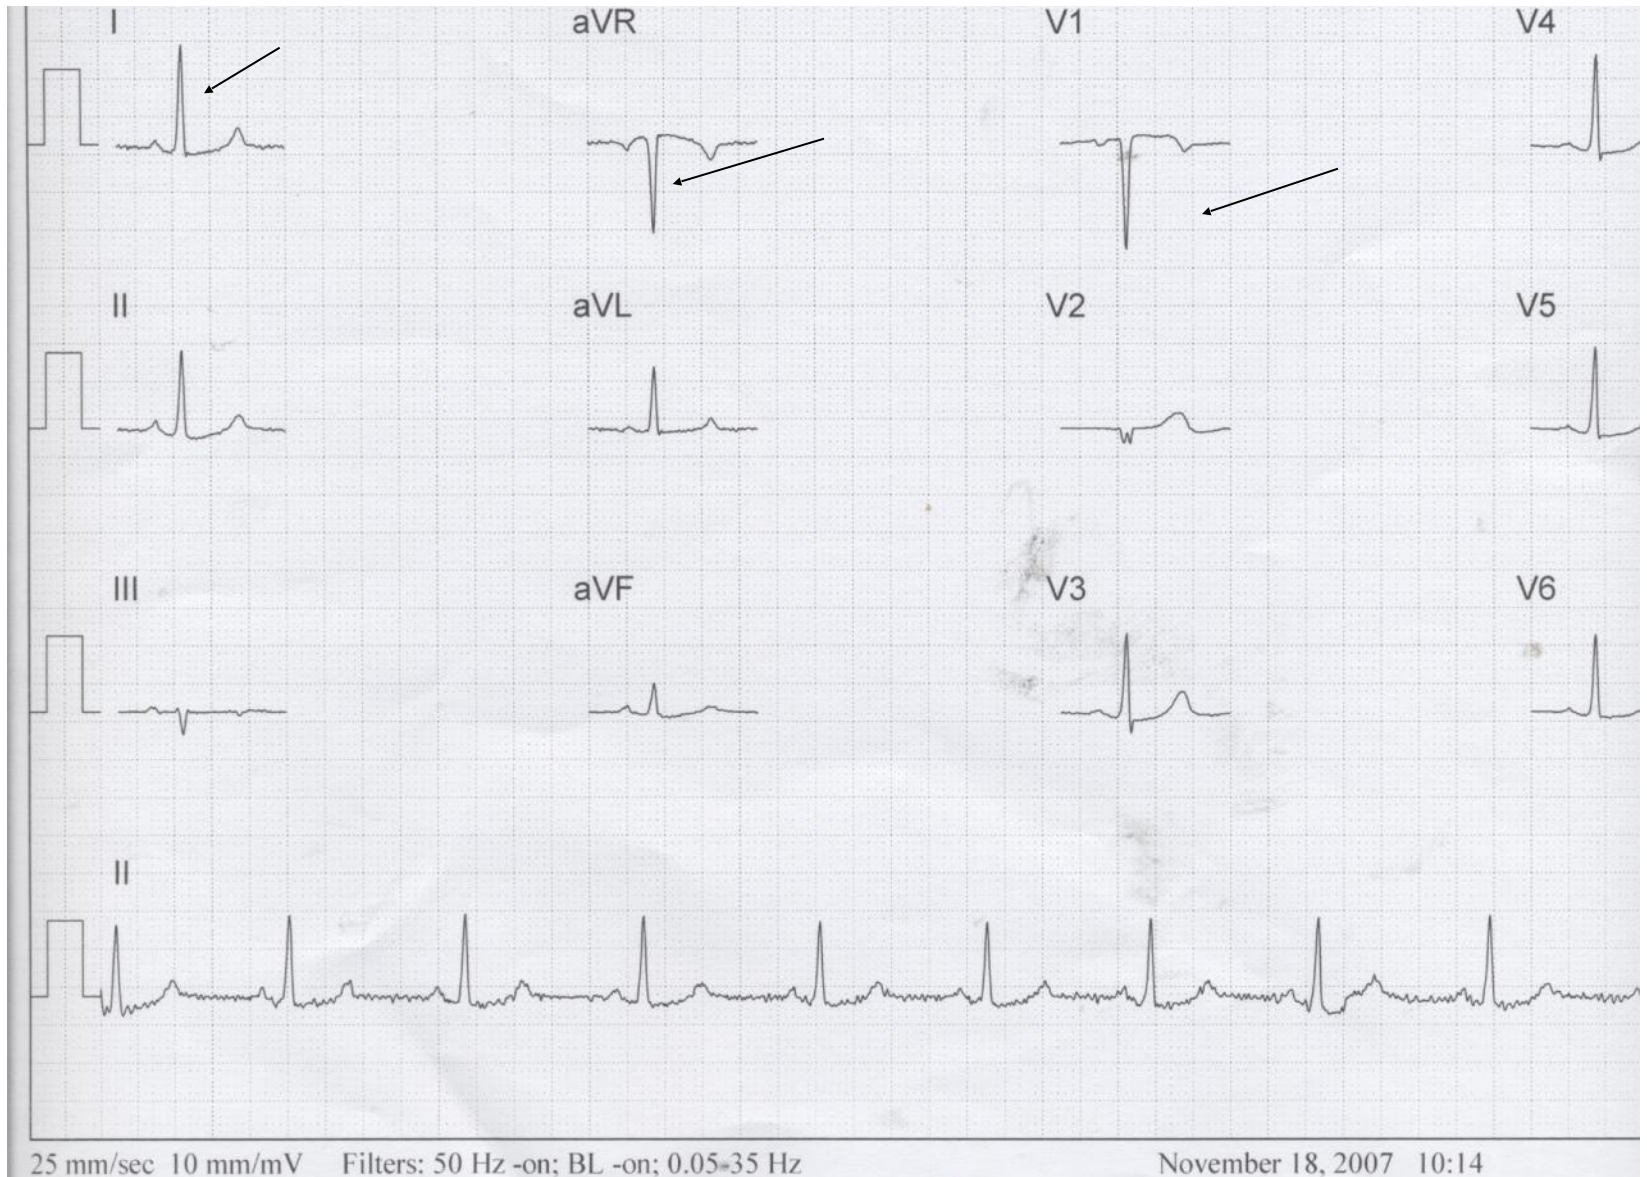

BT009239773,F, 85,HT,

posterior

